


Time-resolved absorption spectrum analysis system

Measure the transient absorption spectrum in extremely short time !

Analysis of the formation and decay process of a reactive intermediate in a photoreaction in solutions, solids, membranes, etc., are possible.

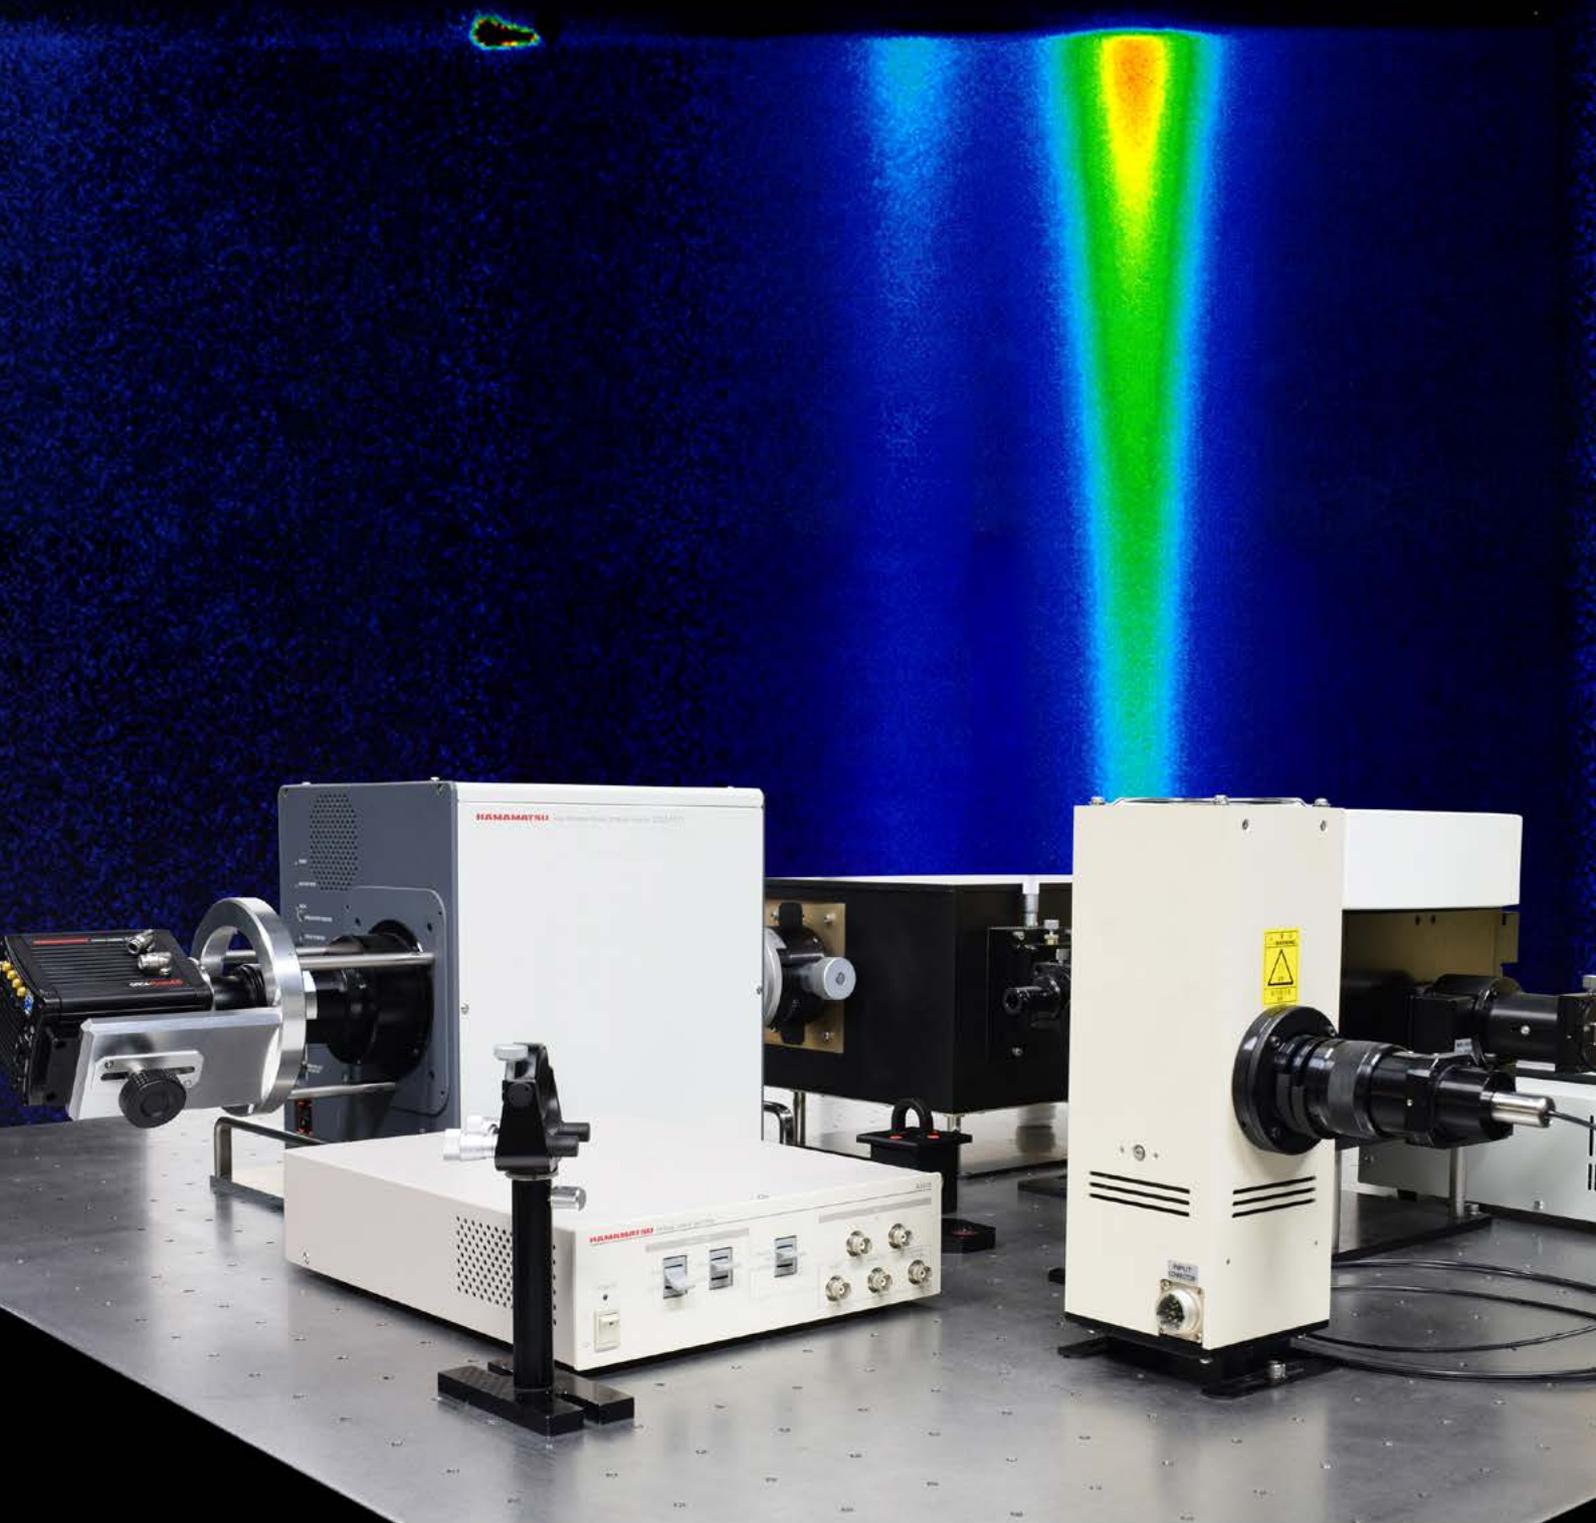

Measure the transient absorption spectrum in extremely short time in a high dynamic range with high S/N.




The time-resolved absorption spectrum analysis system is a device to perform transient absorption spectrum measurements in extremely short time. This system enables to analyze the formation and decay process of a reactive intermediate in a photoreaction in solutions, solids, membranes, etc., are possible. By using the streak camera as the detector and performing multiple-wavelengths time-resolved measurements with a single shot, time-resolved absorption spectra and transient absorption time-resolved spectral images can be measured simultaneously, and you can obtain images of irreversible phenomenon. The newly developed High dynamic range streak camera C13410-01A is employed as the detection device. Minute transient absorption changes can also be measured in a high dynamic range with high S/N.

Features

- **Measurements with the smallest optical density (OD) of 0.005 (for single shot, OD value is 0.02 or less)**
- **Simultaneous measurements of multiple wavelengths using a single shot**
- **High time resolution**
- **Automatic measurements with computer control**

System configuration

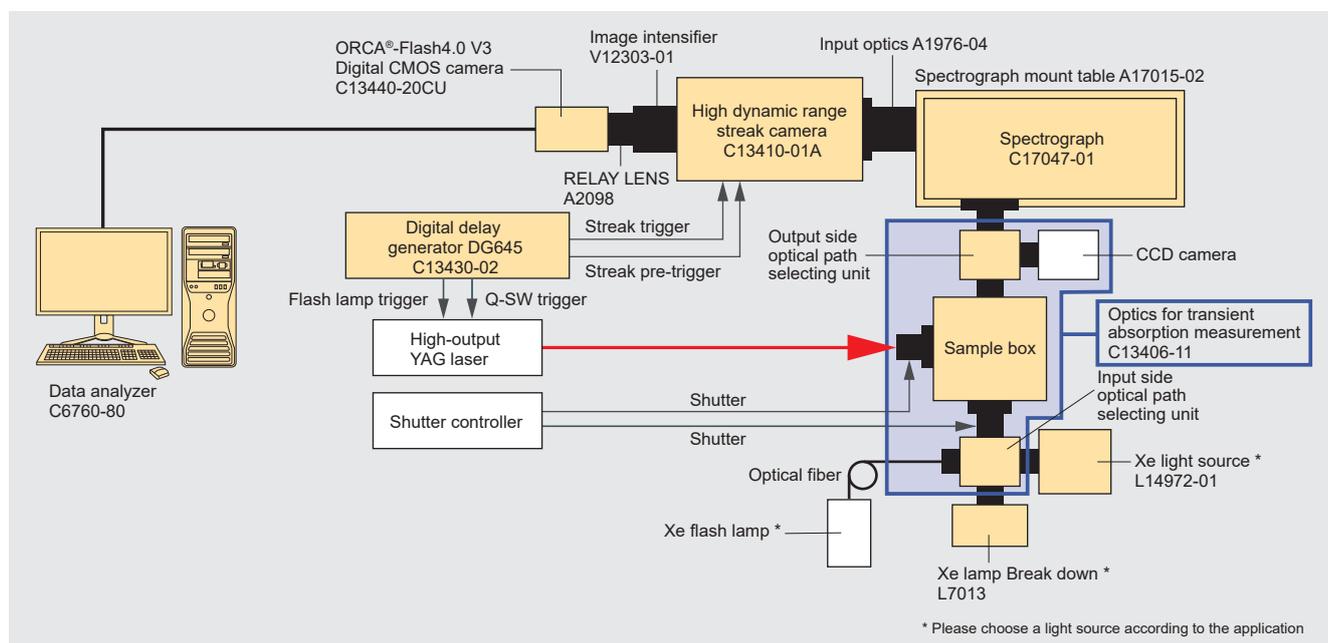

General performance

Specifications

| | Nanosecond Q-SW YAG laser | Picosecond mode-lock YAG laser |
|---|--|--------------------------------|
| Temporal resolution | <7 ns | <70 ps |
| Measurement time range | 20 ns to 1 ms | 0.5 ns to 20 ns |
| White light source | Xe lamp 150 W/CW | Xe lamp Break down |
| Measurement OD value | 0.005 (for single shot, 0.02 or less) | |
| Simultaneous observation wavelength width (W) and wavelength resolution ($\Delta\lambda$) | 100 gr/mm: W= 510 nm, $\Delta\lambda$ <3.0 nm | |
| | 150 gr/mm: W= 340 nm, $\Delta\lambda$ <2.0 nm | |
| | 300 gr/mm: W= 170 nm, $\Delta\lambda$ <1.0 nm | |
| | 600 gr/mm: W= 85 nm, $\Delta\lambda$ <0.5 nm | |
| Measurement wavelength range | 250 nm to 750 nm | |
| Number of channels | Time axis: 1016 ch Wavelength axis: 1344 ch | |

Functions

The time-resolved absorption spectrum analyzing system is composed of a pump and probe lights, optics including shutters (a streak camera transient absorption measurement optical system), a detector part (a spectrograph, a high dynamic range streak camera, and high sensitive digital camera), delay generators, and a data analyzer. For example, a high-output Xenon lamp and a nano-second Q-SW YAG laser are utilized as the pump and probe lights respectively. The pump and probe lights are operated the shutters on the transient absorption measurement software in the data analyzer, and time resolved images such as Data Monitor, (Emission) and Dark images are measured by the detector part.

Transient absorption image is obtained from the time-resolved images by calculation with analysis functions.

Control functions

- Streak camera : time range, MCP gain
- Spectrograph : grating selection, central wavelength setting, slit width setting
- Shutter : shutter opening and closing for excitation light and white light
- Delay generator : delay value setting

Display functions

- Transient absorption time-resolved spectral images
- Transient absorption time and wavelength profiles

Data storage functions

Live image data (Data, Monitor, Emission1, Emission2, Dark, Absorption1, and Absorption2 from the dialog box), spectrum profiles, and time profiles can be saved as files. This does not include fitting data.


- Image file format : TIFF, ITEX
- Profile file format : TEXT file

Analysis functions

- Analyzing transient absorption operation images
 - For nonfluorescent samples
Absorption1= $-\log_{10} ([Date-Dark]/[Monitor-Dark])$
 - For fluorescent samples
Absorption2= $-\log_{10} ([Date-Emission]/[Monitor-Dark])$
- Analyzing fluorescence images from Emission2
Emission2=Emission1-Dark

Measurement functions


- Data measurements
(The white light is measured with both the pump light and probe light shutters open.)
- Monitor measurements
(The white light is measured with only the probe light shutter open.)
- Emission measurements
(The fluorescence is measured with only the pump light shutter open.)
- Dark measurements
(The dark current is measured with both the pump light and probe light shutters closed.)

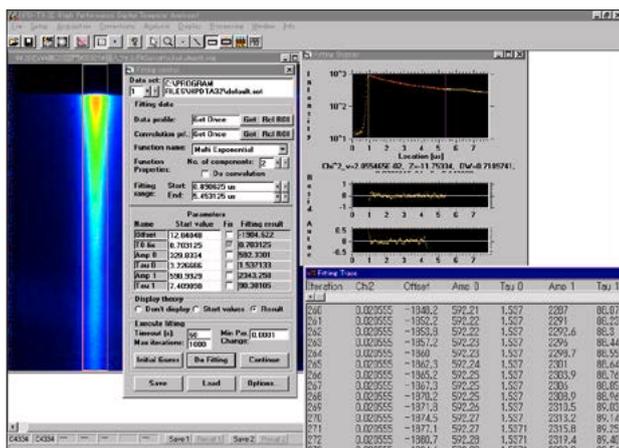

Absorption2
Transient absorption operation image, example of transient spectrum profile display

Operating principle

Using a streak camera as the detector

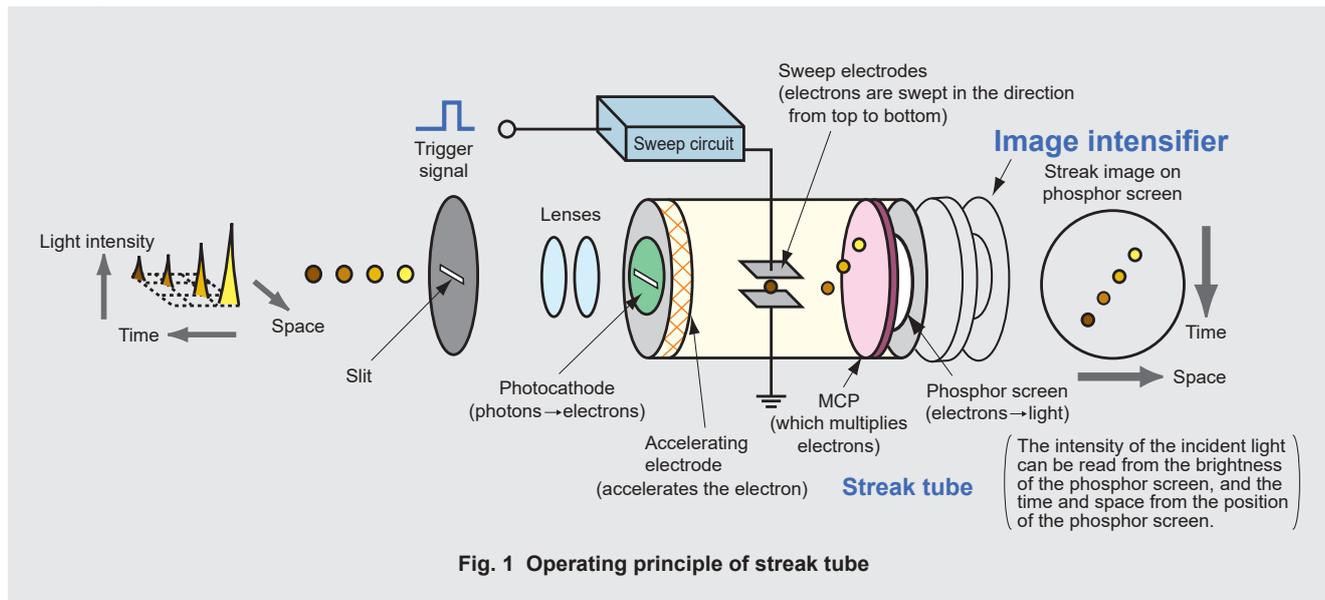

Streak camera operating principle

The streak camera is a device that measures and displays the temporal variations of the incident light intensity as the luminance distribution using the positions (spatially) on the screen by converting incident light into electrons and performing a high speed sweep of the electrons from top to bottom. Fig. 1 shows the operating principle of the streak tube at the heart of the streak camera.

The light pulse being measured passes through the slit and the lenses and the image of the light is formed as the slit image on the photocathode of the streak tube. Supposing now, there is a slight lag both temporally and spatially and four light pulses with different light intensities pass through the slit before reaching the photocathode. Because the photocathode also converts the light pulses into electrons proportional to the intensity of the incident light, the four light pulses are converted into electrons in order and accelerated by the accelerating electrode before being conducted towards the phosphor screen. The high-speed sweeping is performed by applying high voltage to the sweep electrodes, timed to the passage between the electrodes of the groups of electrons created from the four light pulses. Because each successive group of electrons arrives a bit later than the previous group, they are deflected at slightly different angles in the perpendicular direction and then bombarded against the phosphor screen where they are converted back into light.

The streak image obtained on the phosphor screen through the image intensifier can be read by a digital camera that has been enhanced for light intensity. The fluorescence image of the first incident light pulse is positioned at the top of the phosphor screen with successive light pulses appearing lower on the screen in order. In other words, the perpendicular direction on the phosphor screen serves as the time axis. In

addition, the brightness of each fluorescence image is proportional to the intensity of the corresponding incident light pulse. The horizontal positions of the fluorescence images correspond to the horizontal positions of the incident light.

Therefore, the spectral images by the spectrograph are formed on the photocathode and the temporal variations in the light intensity that occur in each wavelength can be measured by performing the streak sweep.

Simultaneous measurements of multiple wavelengths

As explained in the "Streak camera operating principle" section, time-resolved spectrum measurements of multiple wavelengths can be performed simultaneously by combining the C13410-01A with the spectrograph. Fig. 2 shows an example of a three-dimensional display of time-resolved spectrum photometry.


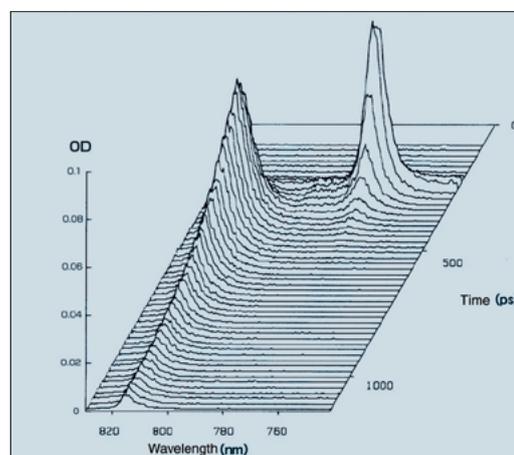


Fig. 2 Example of a three-dimensional display of time-resolved spectrum photometry

Measurement example


Measurement of transient absorption time-resolved spectrum

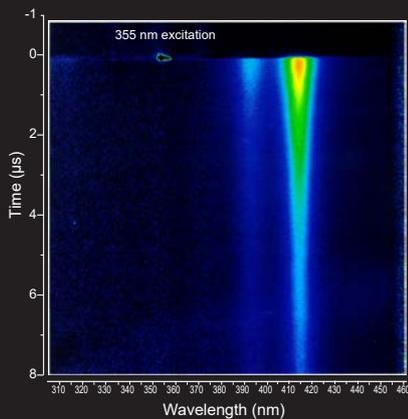


Time-resolved transient absorption spectral streak image of the triplet-triplet absorption of anthracene in supercritical carbon dioxide (40 °C, 10.9 MPa)

Data courtesy of:
National Institute of Advanced Industrial Science and Technology
Supercritical Fluid Research Center (Sendai City, Japan)


Researcher:
Dr. Takafumi Aizawa

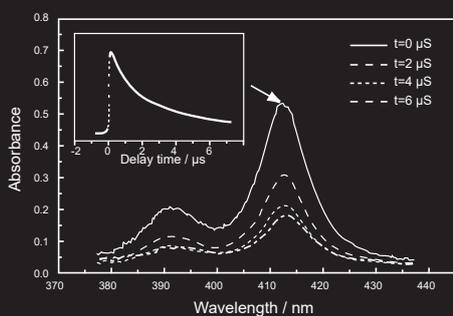

Triplet-triplet absorption spectral of anthracene in supercritical carbon dioxide (40 °C, 10.9 MPa)

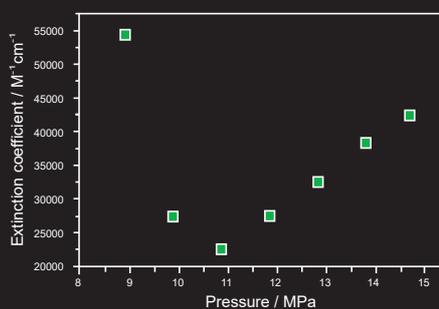


Pressure dependency of the molar extinction coefficient of triplet anthracene (40 °C)

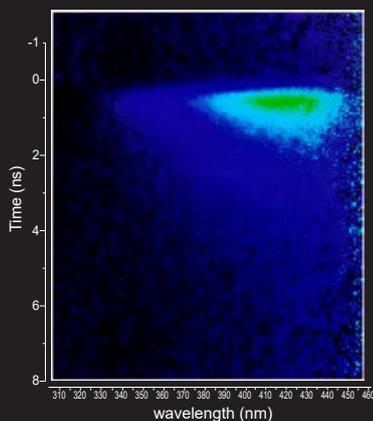


Time-resolved transient absorption spectral streak image of the singlet-singlet absorption of C60

Data courtesy of:
Tohoku University, Institute for Chemical Reaction Science
Professor Osamu Ito

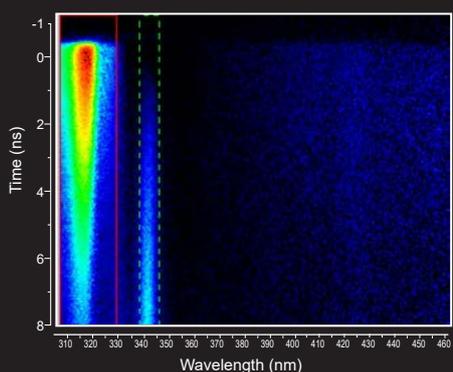

Time-resolved transient absorption spectral streak image in simultaneous observation of the singlet-singlet absorption and the triplet-triplet formation of Anthracene solution

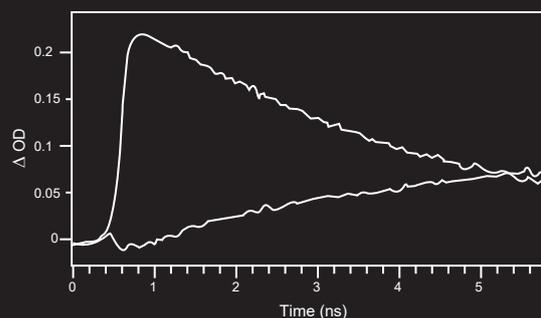

Specifications

High dynamic range streak camera C13410-01A

The streak camera is an ultra high-speed detector with 5 ps temporal resolution. By combining with the spectrograph, transient absorption spectrums can be measured using with a single shot because multiple wavelengths can be observed simultaneously.



| | | |
|-------------|------------------------------------|---|
| Streak tube | Photocathode | S-20 |
| | Spectral response | 200 nm to 850 nm |
| | Effective photocathode size | 7.0 mm (W) × 17.48 mm (L) |
| | Phosphor screen | P-43, Φ25 mm, Fiberoptic output |
| | Image enhancement part | Image Intensifier (I.I.) / Image Booster (I.B.) Outside attachment |
| Main unit | Temporal resolution | Better than 5 ps (at the fastest sweep range) |
| | Sweep time/full screen 1,2,5 step | 0.5 ns to 1 ms |
| | Trigger jitter | Less than ± 20 ps (at the fastest sweep range) |
| | Trigger delay | Approx. 30 ns (at the fastest sweep range) |
| | Maximum sweep repetition frequency | 1 kHz at OPEN FIXED mode, 100 Hz at NORMAL mode |

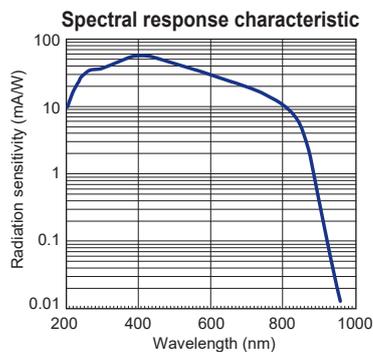


Image intensifier V12303-01

The image intensifier is an option to enhance the streak image at the phosphor screen of the streak tube about 3000 times and output it.



| | |
|----------------|-------------|
| Photocathode | Bialkali |
| Luminance gain | 3100 (typ.) |
| MCP | Built-in |

ORCA®-Flash4.0 V3 Digital CMOS camera C13440-20CU

Recommended readout camera for universal applications, including single-shot, analog and photon counting integration.



| | |
|----------------------------------|--|
| Effective number of pixels | 2048 (H) × 2048 (V) |
| Number of pixels on working area | 1280 (H) × 968 (V) |
| Pixel size | 6.5 μm (H) × 6.5 μm (V) |
| Effective area | 13.312 mm (H) × 13.312 mm (V) |
| Frame rate | 100 frames/s Standard scan (Full resolution, Camera Link) |
| Working area on phosphor screen | 17.47 mm (H) × 13.21 mm (V) |
| Exposure time | 1 ms to 10 s Standard scan Internal trigger mode with Full resolution |
| Digital output | 16 bit |

Spectrograph C17047-01

The spectrograph is ideally suited for combination with the streak camera. Since an optical system that corrects for astigmatism is used, the light condensing efficiency at the detector is high and high-sensitivity measurements are possible.



| | |
|---------------------------|----------------------------------|
| Optical layout | Czerny-Turner model |
| Focal distance | 193 mm |
| F value | 3.6 |
| Incident light slit width | Variable between 10 μm to 2.5 mm |
| Grating | 2 |
| Reciprocal dispersion | 3.53 nm/mm |

•Gratings (typical examples)

| Product number | Number of lines | Blaze wavelength | Measurement wavelength range | Wavelength resolution |
|----------------|-----------------|------------------|------------------------------|-----------------------|
| A17048-010-078 | 100 L/nm | 780 nm | Approx. 868 nm | Approx. 13 nm |
| A17048-015-050 | 150 L/nm | 500 nm | Approx. 570 nm | Approx. 8.6 nm |
| A17048-030-050 | 300 L/nm | 500 nm | Approx. 281 nm | Approx. 4.2 nm |
| A17048-060-050 | 600 L/nm | 500 nm | Approx. 136 nm | Approx. 2.0 nm |

* These are the values when using ORCA®-Flash4.0 V3 as a readout camera.

Spectrograph mount table A17015-02

The spectrograph mount table is a support stand for connecting and fixing the spectrograph and streak camera.

Digital delay generator DG645 C13430-02

The DG645 is a general-purpose delay generator that matches the streak camera timing with the pulsed laser timing, mainly for slower streak times.



| | |
|---------------------------|---------------------------------------|
| Number of output channels | 4 ch (AB, CD, EF, GH output terminal) |
| Output level | 0.5 V to 5.0 V 50 Ω |
| Variable delay range | 0 ps to 2000 s |
| Delay resolution | 5 ps |
| Internal delay time | 85 ns |
| Repetition rate | Single to 10 MHz |
| Jitter | < 25 ps rms |
| Interface | GPIB/RS-232C |

Delay unit C15936

The delay unit is used to adjust the operation timing of streak camera with the laser pulse.



| | |
|---------------------|---|
| Delay range | 0 ns to 31.96 ns |
| Delay setting range | 30 ps, 60 ps, 120 ps, 250 ps, 500 ps, 1 ns, 2 ns, 4 ns, 8 ns, 16 ns |

Optics for transient absorption measurement C13406-11


The optics for transient absorption measurement contains 3 kinds of optics: a white light input optics, an excitation optics, and 2 optical laser shutters.

Measurements can be performed accurately in the 250 nm to 750 nm measurement wavelength range. Excitation optics is composed of 2 YAG laser mirrors with wavelength 266 nm, 355 nm, and 532 nm respectively.

| | |
|------------------------------|---|
| Measurement wavelength range | 250 nm to 750 nm |
| Laser mirror | Dielectric multilayer mirror (for 266 nm, 355 nm, 532 nm) |
| Sample holder | 10 mm cell holder, 2 mm cell holder, Thin film sample holder |
| Laser shutter (A6538) | Rotating solenoid, 2 heads (1 for pump light / 1 for probe light) |

Xe light source L14972-01

The Xe light source is a highly stable white light source without shaking or movement at the source of the arc light.

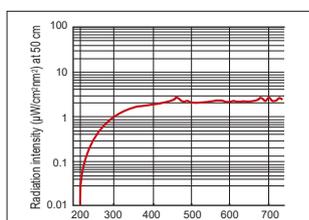

| | |
|------------------------|--|
| Radiation wavelength | 220 nm to 2000 nm |
| Radiation intensity | 250 nm : 0.52 $\mu\text{W}/\text{cm}^2 \cdot \text{nm}^{-1}$ at 50 cm 500 nm : 2.00 $\mu\text{W}/\text{cm}^2 \cdot \text{nm}^{-1}$ at 50 cm |
| Power consumption | 150 W |
| Window material | Ozoneless quartz |
| Light output stability | Drift : $\pm 0.5\%$ /h (typ.) Fluctuation : 1.0 % (Max.) |

Xe lamp Break down L7013

The Xe lamp Break down can generate extremely bright white light from 250 nm to 750 nm with 50 ns pulse width (FWHM) by focusing the fundamental wavelength (1064 nm) of the high output picosecond laser onto the Xe cell.



This is different from ordinary pulse xenon lamps and allows you to obtain smooth spectra without bright lines. By combining with a high-output picosecond laser, transient absorption measurements are possible in the picosecond region.

| | |
|---------------------------|---|
| Emission wavelength range | 250 nm to 750 nm |
| Emission time width | Approx. 50 ns (FWHM) |
| Stability | OD corresponding value less than ± 0.005 *1 |
| Noise | OD corresponding value less than ± 0.02 *2 |

*1 This is the baseline shaking when the absorption operation is performed and was determined from two single shot measurements of the white light output when a 20 mJ/pulse YAG laser light was directed at the L7013.

*2 This is the noise level when the absorption operation is performed and was determined from a single shot measurement of the white light under the same conditions as in.

Excitation light source

The YAG laser is the excitation light source for transient absorption measurements. The system can be enhanced by combining with the lasers from various manufacturers.

Data analyzer C6760-80

The data analyzer is used to control each device such as the streak camera and spectrograph and to collect and analyze data.

| | |
|------------------|--|
| Supported camera | ORCA®-Flash4.0 V3 Digital CMOS camera C13440-20CU |
| Component | Computer set Software HPD-TA + Ta-Abs Frame grabber board DIO board External trigger cable Shutter cable Camera Link cable |
| System | Windows® 11 Pro |
| Interface | Camera Link |

<Control & readout software HPD-TA> * Including in the Data analyzer

| | |
|-------------------------|---|
| Data acquisition | Live mode, Analog integration mode Photon counting mode, Sequence recording mode |
| Device control | Streak camera, Readout camera, Spectrograph, Delay units |
| Profile function | Real-time display, min/max, FWHM, Gauss fit |
| Data corrections | Background, Sensitivity, Curvature, Jitter |
| Axis calibration | Channel, Time, Wavelength |
| File formats (images) | Binary (up to 32 bit), TIFF, ASCII |
| File formats (profiles) | ASCII |

Laser handling mirror for T-Absorption A8005 (optional)

The laser handling mirror is used to direct the YAG laser in the optical system.


| | |
|-----------------------|---|
| Coating | Dielectric multilayer film mirror |
| Reflection wavelength | 266 nm, 355 nm, 532 nm and 1.06 μm |

Coaxial excitation optics (optional)


This is an optical system to excite the excitation light on the same axis as the white light. The excitation light is reflected by the dichroic mirror and is directed at the sample on the same axis. This excitation light is removed by the color filter installed after the sample. This optical system is used to perform transient absorption measurements of solution samples, film, and membrane samples in a cell with a 2 mm optical path length.

Dimensional outlines (Unit: mm)


● **High dynamic range streak camera C13410-01A (Approx. 26 kg Main unit only)**

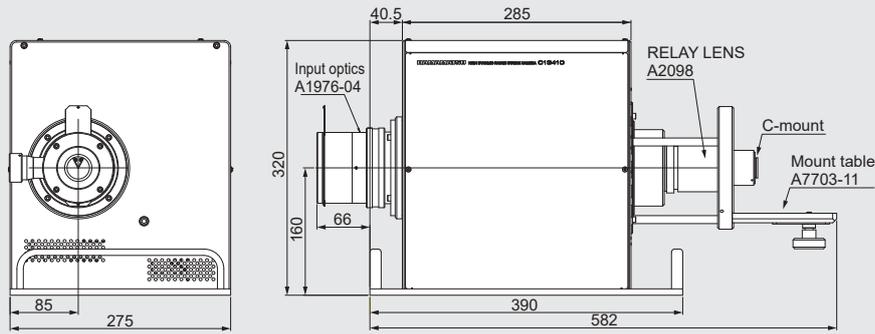


● **Spectrograph C17047-01 f=193 mm (Approx. 7.5 kg)**

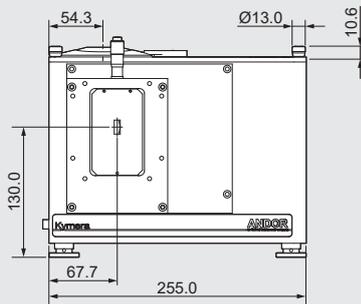

● **ORCA®-Flash4.0 V3 Digital CMOS camera C13440-20CU (Approx. 2.2 kg)**

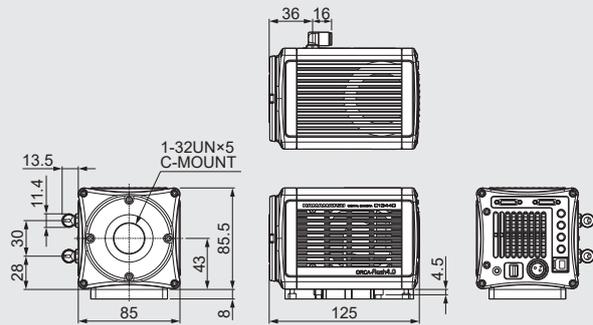

● **Optics for transient absorption measurement C13406-11 (Approx. 18 kg)**

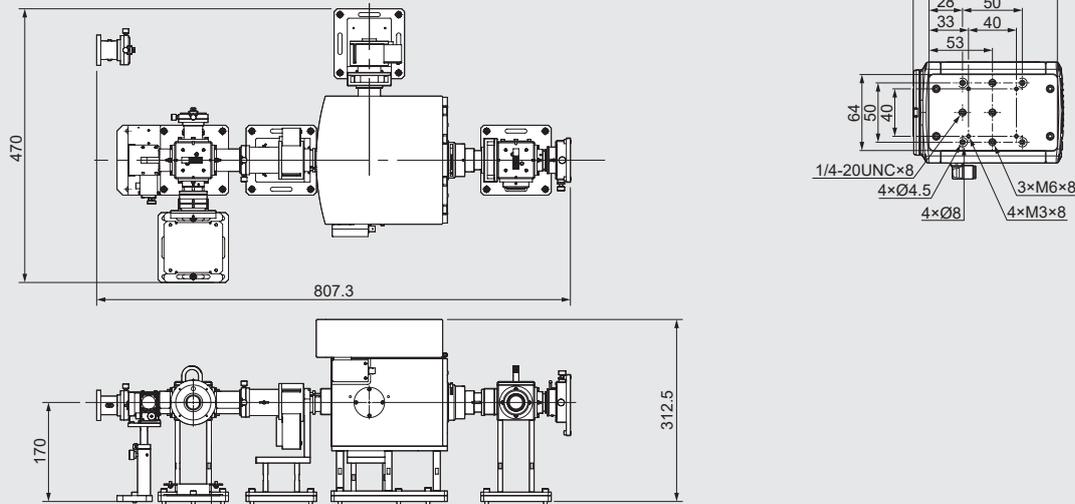

- ORCA is a registered trademark of Hamamatsu Photonics K.K. (China, EU, France, Germany, Japan, UK, USA).
 - Windows is a registered trademark of Microsoft Corporation in the USA (and other countries).
 - The product and software package names noted in this brochure are trademarks or registered trademarks of their respective manufacturers.
 - Subject to local technical requirements and regulations, availability of products included in this brochure may vary. Please consult your local sales representative.
 - The products described in this brochure are designed to meet the written specifications, when used strictly in accordance with all instructions.
 - The university, institute, or company name of the researchers, whose measurement data is published in this brochure, is subject to change.
 - The spectral response specified in this brochure is typical value and not guaranteed.
 - The measurement examples in this brochure are not guaranteed.
 - Specifications and external appearance are subject to change without notice.
- © 2024 Hamamatsu Photonics K.K.

HAMAMATSU PHOTONICS K.K. www.hamamatsu.com

Systems Division

812 Joko-cho, Chuo-ku, Hamamatsu City, 431-3196, Japan, Telephone: (81)53-431-0124, Fax: (81)53-433-8031, E-mail: export@sys.hpk.co.jp

U.S.A.: HAMAMATSU CORPORATION: 360 Foothill Road, Bridgewater, NJ 08807, U.S.A., Telephone: (1)908-231-0960, Fax: (1)908-231-1218

Germany: HAMAMATSU PHOTONICS DEUTSCHLAND GMBH: Arzbergerstr. 10, 82211 Herrsching am Ammersee, Germany, Telephone: (49)8152-375-0, Fax: (49)8152-265-8 E-mail: info@hamamatsu.de

France: HAMAMATSU PHOTONICS FRANCE S.A.R.L.: 19 Rue du Saule Trapu, Parc du Moulin de Massy, 91882 Massy Cedex, France, Telephone: (33)1 69 53 71 00, Fax: (33)1 69 53 71 10 E-mail: infos@hamamatsu.fr

United Kingdom: HAMAMATSU PHOTONICS UK LIMITED: 2 Howard Court, 10 Tewin Road, Welwyn Garden City, Hertfordshire, AL7 1BW, UK, Telephone: (44)1707-294888, Fax: (44)1707-325777 E-mail: info@hamamatsu.co.uk

North Europe: HAMAMATSU PHOTONICS NORDEN AB: Torshamnsgatan 35 16440 Kista, Sweden, Telephone: (46)8-509 031 00, Fax: (46)8-509 031 01 E-mail: info@hamamatsu.se

Italy: HAMAMATSU PHOTONICS ITALIA S.R.L.: Strada della Moia, 1 int. 6, 20044 Arese (Milano), Italy, Telephone: (39)02-93 58 17 33, Fax: (39)02-93 58 17 41 E-mail: info@hamamatsu.it

China: HAMAMATSU PHOTONICS (CHINA) CO., LTD.: 1201 Tower B, Jiaming Center, 27 Dongsanhuan Beilu, Chaoyang District, 100020 Beijing, P.R. China, Telephone: (86)10-6586-6006, Fax: (86)10-6586-2666 E-mail: hpc@hamamatsu.com.cn

Taiwan: HAMAMATSU PHOTONICS TAIWAN CO., LTD.: 13F-1, No.101, Section 2, Gongdao 5th Road, East Dist., Hsinchu City, 300046, Taiwan(R.O.C), Telephone: (886)3-659-0080, Fax: (886)3-659-0081 E-mail: info@hamamatsu.com.tw

Cat. No. SHSS0005E07
MAR/2024 HPK
Created in Japan